



Three-dimensional imaging for indirect-direct bonding

Ahmed M. El-Timamy,^a Fouad A. El-Sharaby,^b Faten H. Eid,^c and Yehya A. Mostafa^c

Cairo and New Cairo, Egypt

The aim of this article is to introduce a new concept of bracket positioning with special consideration to root axes. Cone-beam computed tomography imaging and computer-aided manufacturing were used to produce stereolithographic trays for indirect-direct bonding. (Am J Orthod Dentofacial Orthop 2016;149:928-31)

Since the evolution of the straight-wire appliance, attention has been directed to precise bracket placement as the key factor for ideal tooth positioning.¹ Accurate bracket positioning enables the clinician to achieve the best treatment outcome in the shortest time and to minimize the need for further arch-wire bending and bracket repositioning. Various utilities have been developed for precise bracket placement along with techniques for indirect bonding.^{2,3}

The frequency of innovations in the design of bracket placement gauges to facilitate accurate bracket positioning is unprecedented. Although these gauges can minimize bracket positioning errors, they cannot negate them.^{4,5} Problems encountered during bracket positioning include inaccessibility, anatomic variations, and morphologic diversity of the clinical crowns, even for the same tooth. Above and beyond is the traditional use of the long axis of the clinical crown as a guide for bracket placement, as dictated by the straight-wire technique,⁶ which was reported to be different from the actual long axis of the tooth when the root was considered.⁷⁻⁹ The ability to align teeth considering both the crown and the root improves the treatment outcome and decreases the chances for posttreatment relapse.

Others have attempted to discover the best method for bracket placement.^{3,10,11} Unfortunately, none has succeeded in reporting a reproducible and reliable technique.^{12,13} Indirect bonding techniques were introduced to prevent the difficulties of inaccessibility and lengthy appointments while obtaining standard results, yet the human factor in bracket placement cannot be overlooked. Many factors might affect the clinician's precision in bracket positioning. These include years of experience, sharpness of sight, and manual dexterity.¹⁴ The evolution of imaging techniques has opened new horizons for both diagnosis and treatment. Recent imaging techniques have allowed complete visualization of the tissues in 3 dimensions.¹⁵ Cone-beam computed tomography (CBCT) has proven to have great diagnostic value,^{15,16} with the ability to produce accurate images of the patient's soft and hard tissues.¹⁷ Furthermore, computer-aided manufacturing of dental stents derived from cone-beam images has a satisfactory degree of accuracy, allowing the implementation of CBCT technology not only as a diagnostic tool but also as a treatment aid.¹⁸

MATERIAL AND METHODS

Three-dimensional (3D) images for separate brackets in a bracket kit (Roth 0.022 in; American Orthodontics, Sheboygan, Wis) were obtained from CBCT scanning. The images were first obtained in DICOM format and then converted to stereolithography format using Mimics software (Materialise, Leuven, Belgium). Stereolithography is a file format that is supported by many other software packages and is widely used for 3D printing and computer-aided manufacturing. Another CBCT image was obtained for the patient (CRANEX 3D; Soredex, Charlotte, NC) with the following parameters: resolution (voxel size), 0.3/0.3 mm; exposure time, 4860 msec; anode voltage,

^aAssistant lecturer, Department of Orthodontics and Dentofacial Orthopedics, Faculty of Oral and Dental Medicine, Cairo University, Cairo, Egypt.

^bLecturer, Department of Orthodontics and Dentofacial Orthopedics, Faculty of Oral and Dental Medicine, Cairo University, Cairo, Egypt.

^cChairman, Department of Orthodontics, Future University in Egypt, New Cairo, Egypt.

All authors have completed and submitted the ICMJE Form for Disclosure of Potential Conflicts of Interest, and none were reported.

Address correspondence to: Fouad A. El-Sharaby, Department of Orthodontics and Dentofacial Orthopedics, Faculty of Oral and Dental Medicine, Cairo University, Saraya El-Manial St, Manial, Cairo, Egypt; e-mail, fouadsharaby@gmail.com.

Submitted, August 2015; revised and accepted, December 2015.
0889-5406/\$36.00

Copyright © 2016 by the American Association of Orthodontists.
<http://dx.doi.org/10.1016/j.ajodo.2015.12.009>

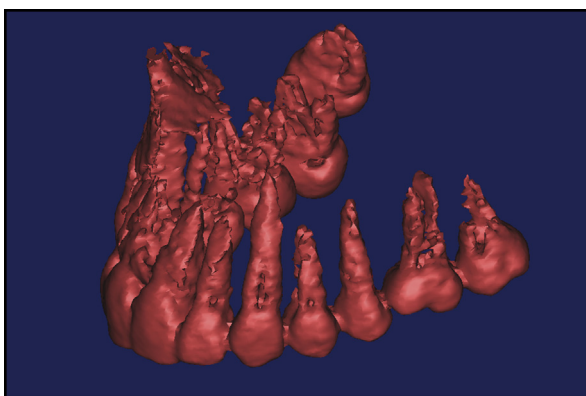


Fig 1. Preparation of patient's CBCT image to isolate the teeth with their roots.

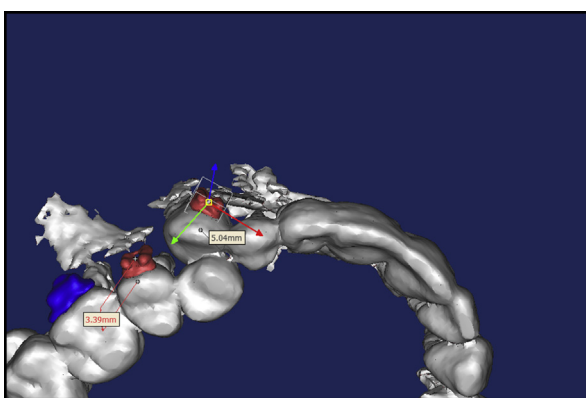


Fig 2. Placement of the brackets with the Mimics software.

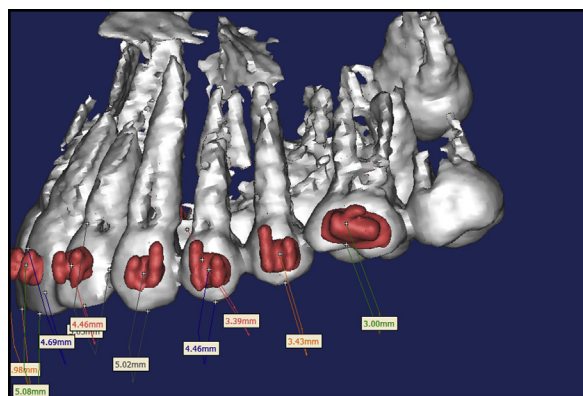


Fig 3. Accurate bracket placement with visualization of the roots.

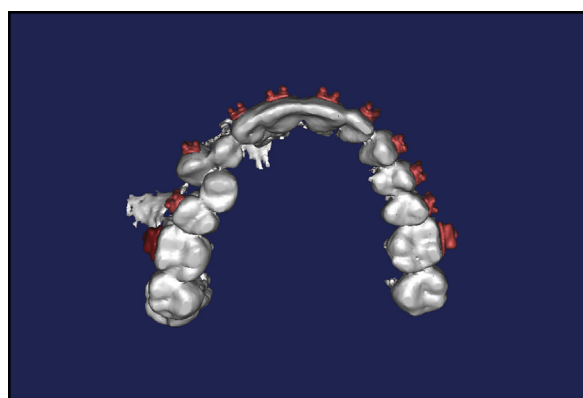


Fig 4. Occlusal view of bracket placement and checking of each bracket.

89.8 kV; field of view, 8°-8 cm; anode current, 10 mA; and sensor, CCD detector. The image was saved in DICOM format and the placed into the Mimics image processing software.

With the thresholding option, the images were enhanced, and the teeth were isolated to gain a clear view of their roots (Fig 1). With both images in the Mimics image-processing software, each bracket was placed on its designated tooth and positioned accurately using the Mimics software tools. The ability to clearly visualize both the crown and the root of every tooth together with precise dimensional measurements allowed for accurate positioning of the brackets, with particular attention to the root axes, aiming for root parallelism at the end of the treatment (Figs 2-4).

After the brackets were placed, a 3D image of a U-shaped stent was added to the project. Then the image of the stent was placed over the teeth and half of the brackets, leaving the other half of the brackets

uncovered. In the Mimics software, the teeth and brackets were then subtracted from the image of the tray to have a negative replica. The subtracted image of the tray in stereolithography format was printed with a 3D printer (FORMIGA P110; EOS e-Manufacturing Solutions, Krailling, Germany) to obtain a 3D printed bracket positioning tray with indentations for bracket seating (Figs 5-7). The printer uses additive manufacturing, laser sintering, and 3D printing. In additive manufacturing, components are built in layers by depositing materials guided by the digital 3D design. The material used to construct the stereolithographic tray was polyamide (PA 2200; EOS, Novi, Mich), which is characterized by high strength and stiffness, good chemical resistance, high detail resolution, and biocompatibility. The actual brackets were then conveyed to the printed trays, and the whole assembly was ready for direct bonding in the patient's mouth (Fig 8).

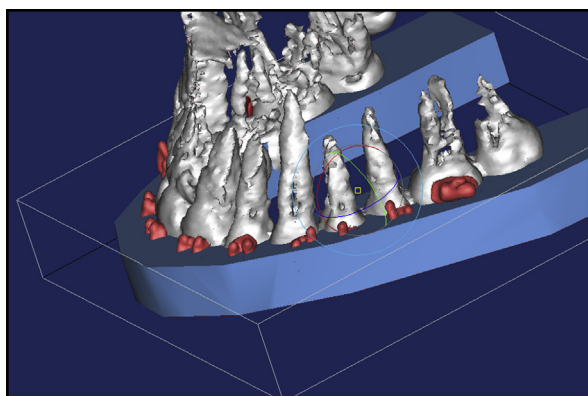


Fig 5. Placement of the U-shaped tray over the brackets and teeth.

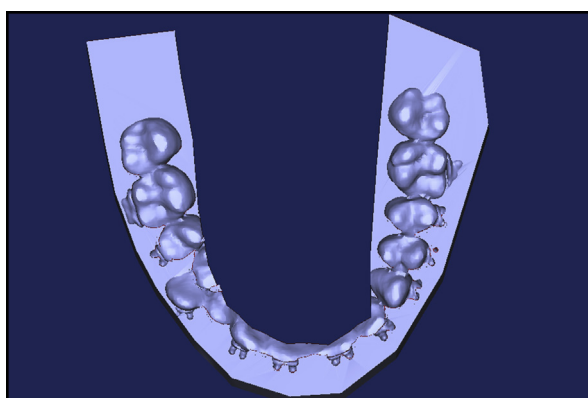


Fig 6. The U-shaped tray after subtraction of the brackets and teeth with the position of the brackets printed inside.

DISCUSSION AND CONCLUSIONS

Implementing contemporary imaging techniques is essential not only for enhancement of the final treatment outcome, but also for both clinician and patient welfare. This technique of indirect-direct bonding will minimize the time, armamentarium, and expenses needed for the preparation of models, trays, and positioning devices for conventional indirect bonding techniques. Moreover, with this technique, brackets will be ready for bonding with virgin bracket bases that are not contaminated with resin or cast material, as is traditionally the case for conventional indirect bonding techniques. Remnants from the cast or excess resin on the bracket base might reduce bond strength or even disrupt the first-order position of the tooth because of the extra bonding material.¹⁹ Additionally, this technique emphasizes root axis consideration during bracket positioning, aiming at accurate posttreatment root parallelism, which is considered essential for posttreatment stability.



Fig 7. The stereolithographic tray after printing.



Fig 8. The stereolithographic tray-bracket assembly ready for bonding.

Having 3D images of brackets from different manufacturers could facilitate their implementation for virtual bonding with this technique without prior need for the 3D scanning step. CBCT imaging together with 3D printing may aid in developing a new technique for precise bracket positioning.

ACKNOWLEDGMENTS

We thank Khalid Abdelghany, Central Metallurgical Research & Development Institute, Cairo, Egypt, for the software support.

REFERENCES

1. Sardarian A, Danaei S, Shahidi S, Boushehri S, Geramy A. The effect of vertical bracket positioning on torque and the resultant stress in the periodontal ligament—a finite element study. *Prog Orthod* 2014;15:50.
2. Koo BC, Chung CH, Vanarsdall RL. Comparison of the accuracy of bracket placement between direct and indirect bonding techniques. *Am J Orthod Dentofacial Orthop* 1999;116:346-51.

3. Milne JW, Andreasen GF, Jakobsen JR. Bond strength comparison: a simplified indirect technique versus direct placement of brackets. *Am J Orthod Dentofacial Orthop* 1989;96:8-15.
4. Ousehal L, Lazrak L. The accuracy of brackets placement in direct bonding technique: a comparison between the pole-like bracket positioning gauge and the star-like bracket positioning gauge. *Open J Stomatol* 2011;1:121-5.
5. Mohammadi A, Moslemzadeh SH. Comparison of the accuracy of bracket placement with height bracket positioning gauge and boone gauge. *J Dent Res Dent Clin Dent Prospects* 2011; 5:111-8.
6. Andrews F. The six keys to normal occlusion. *Am J Orthod* 1972; 62:296-309.
7. Bryant RM, Sadowsky PL, Hazelrig JB. Variability in three morphologic features of the permanent maxillary central incisor. *Am J Orthod* 1984;86:25-32.
8. Dewel BF. Clinical observations on the axial inclination of teeth. *Am J Orthod* 1949;35:98-115.
9. Carlsson R, Rönnerman A. Crown-root angles of upper central incisors. *Am J Orthod* 1973;64:147-54.
10. Joiner M. In-house precision bracket placement with the indirect bonding technique. *Am J Orthod Dentofacial Orthop* 2010;137: 850-4.
11. Carlson SK, Johnson E. Bracket positioning and resets: five steps to align crowns and roots consistently. *Am J Orthod Dentofacial Orthop* 2001;119:76-80.
12. Nichols DA, Gardner G, Carballeyra AD, Marsh CM. Reproducibility of bracket positioning in the indirect bonding technique. *Am J Orthod Dentofacial Orthop* 2013;144:770-6.
13. Shpack N, Geron S, Floris I, Davidovitch M, Brosh T, Vardimon AD. Bracket placement in lingual vs labial systems and direct vs indirect bonding. *Angle Orthod* 2007;77:509-17.
14. Garino F, Garino GB. Computer-aided interactive indirect bonding. *Prog Orthod* 2005;6:214-23.
15. El-Zanaty HM, El-Beialy AR, Abou El-Ezz AM, Attia KH, El-Bialy AR, Mostafa YA. Three-dimensional dental measurements: an alternative to plaster models. *Am J Orthod Dentofacial Orthop* 2010;137:259-65.
16. Cevidanes LH, Styner MA, Proffit WR. Image analysis and superimposition of 3-dimensional cone-beam computed tomography models. *Am J Orthod Dentofacial Orthop* 2006;129:611-8.
17. Tong H, Enciso R, Van Elslande D, Major PW, Sameshima GT. A new method to measure mesiodistal angulation and faciolingual inclination of each whole tooth with volumetric cone-beam computed tomography images. *Am J Orthod Dentofacial Orthop* 2012;142:133-43.
18. Kim SH, Kang JM, Choi B, Nelson G. Clinical application of a stereolithographic surgical guide for simple positioning of orthodontic mini-implants. *World J Orthod* 2008;9:371-82.
19. Thompson MA, Drummond JL, BeGole EA. Bond strength analysis of custom base variables in indirect bonding techniques. *Am J Orthod Dentofacial Orthop* 2008;133:9.e15-20.